

Single channel Load cell

KOSD

KIMD

KISD

Double channel Load cell

KOSD-D

KIMD-D



User manual

Content

General	1
Specifications.....	3
Intrinsic safety	4
Load cell ATEX-label	4
Functional safety.....	5
Load cell connection	6
Application examples	7
Mechanical installation and maintenance	8
Mechanical data.....	8
Appendix 1, 200418r5, Baseefa02ATEX0072	9
Appendix 2, 200706r1, BAS22UKEX0266.....	13
Appendix 3, 200441r8, Declaration of Conformity	16
Appendix 4, IECEx and Functional Safety Certificates	17

PRECAUTIONS

READ this manual BEFORE operating or servicing this unit.
FOLLOW these instructions carefully.
SAVE this manual for future reference.



WARNING

Only qualified personnel are permitted to install and service this unit. Exercise care when making checks, tests and adjustments that must be made with power on.
Failing to observe these precautions could result in bodily harm.

DO NOT allow untrained personnel to operate, clean, inspect, maintain, service, or tamper with this unit.

INTENDED USE

KxxD (-D) line of load cells are intended for industrial systems. Its basic function is force measuring or weighing applications. The strain gauge bridge output wiring is connected to an overall measurement system.

Changes to current manual version

Detailed application, intrinsic safety and functional safety information added.


General

KxxD-(D) is a line of load cells (KOSD-(D), KIMD-(D) and KISD-(D)) with a high degree of protection. They incorporate resistive strain gauges, measuring the shear force or tension.


The KxxD-versions have one electrical circuit and the KxxD-D-version two separate electrical circuits. For the KxxD-D-version the safety parameters are applicable to each circuit individually. The two separate electrical circuits are insulated from each other.

The following KxxD-D load cell configurations are available:


Single bridge load cell with connector or cable connection

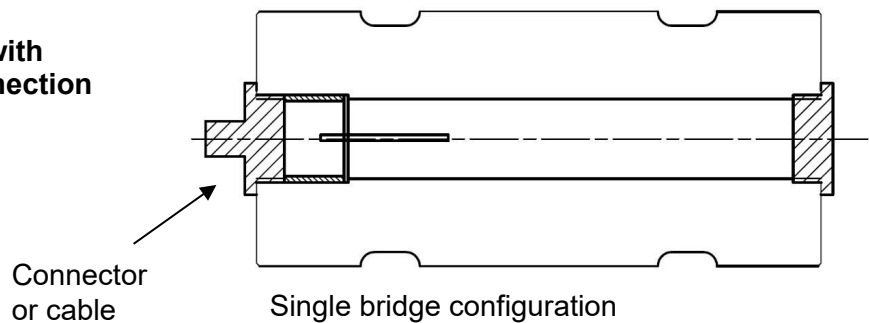

Dual bridge load cell with common connector or common cable connection

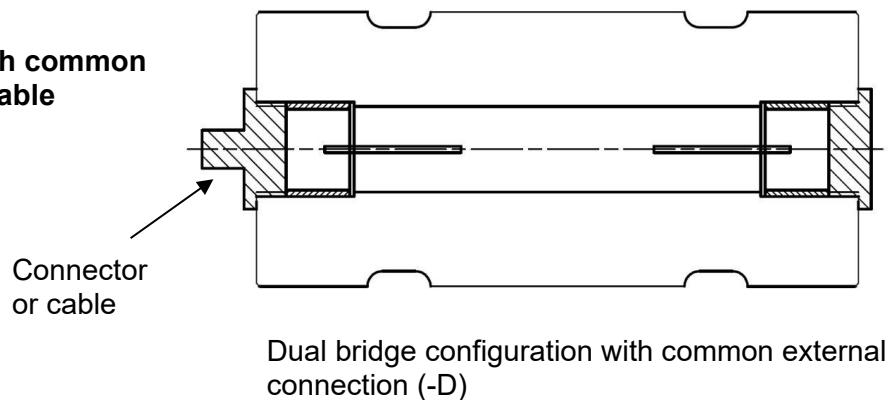

Dual bridge load cell with individual connector or cable connections.

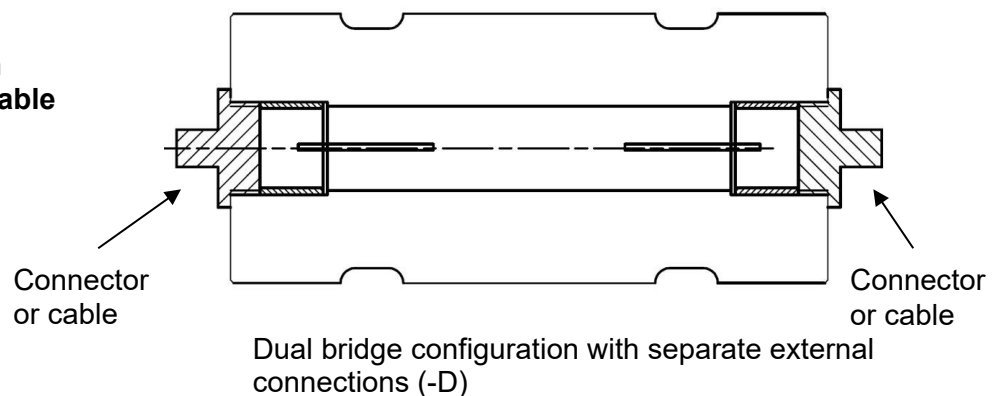

The load cells can be supplied with connector or cable connection (see also page 6 and 7).




4-pin connector



Cable connection

- KxxD with one 4-pin connector or cable
- KxxD-D with one 8-pin connector or cable connection
- KxxD-D with two 4-pin connectors or dual cable connections
- KxxD-D with one 4-pin connector and single cable connection

These load cells are approved for use in an explosive hazardous area, provided that suitable intrinsic safety barriers or insulators are used and no rubbing with electrostatic materials occurs on outside potted cavities surfaces.

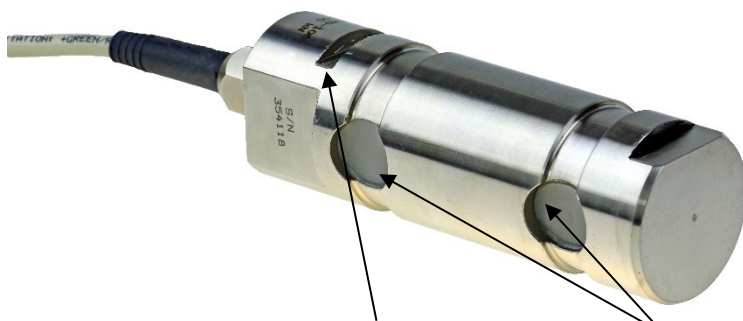

Rotation reference
surface

Potted
cavite

CE-marking and UKEX-marking according to ATEX and EMC Directives, see appendix 1 and 2.

Specifications

Approvals:				
ATEX intrinsic safety	For KxxD-X, Baseefa02ATEX0072 Issue 5, see appendix 1			
	For KxxD-X, BAS22UKEX0266 Issue 1, see appendix 2			
IECEx intrinsic safety	For Kxx(D)-(D) X, IECEx BAS 14.0015X Issue 4, see appendix 4			
Functional safety	TÜV 968/FSP 1462.00/22, see appendix 4			
Environmental conditions:				
PARAMETER	Min.	Typ.	Max.	UNIT
Environmental protection / IP rating		IP67		
Operating Temperature (T _{amb})	-40		+60	°C
System parameters:				
	See LC calibration data sheet			
Load cell strain gauge:				
Impedance		350		Ohm
ATEX conditions:				
Insulation test		500		Vrms
Input parameters	See appendix 1 & 2			

Intrinsic safety

All load cells KxxD (-D) can be approved for use in explosive gas or dust area.


The last 'X' in the type code (see load cell ATEX label) is a number to identify the specific model. They can be ordered either with a cable connector or with an integrated cable. The safety description is labelled on the load cell.

For the -D version, the safety description and connection is applicable to each load cell bridge output.


Internal capacitance and inductance see ATEX approvals.

The cable inductance is negligible compared to the allowed upper limit.


Load cell ATEX-label

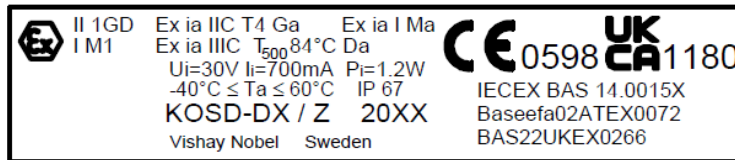


KOSD-D

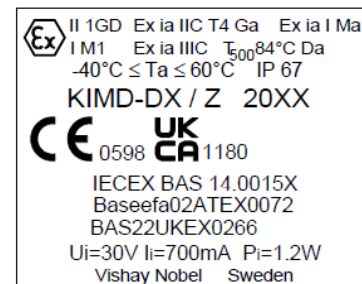


KIMD-D

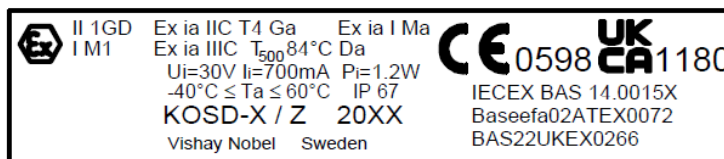

KOSD

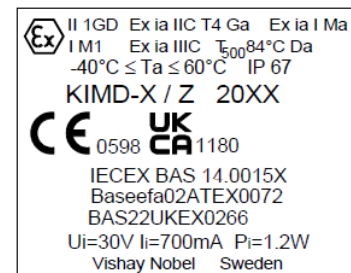

KIMD

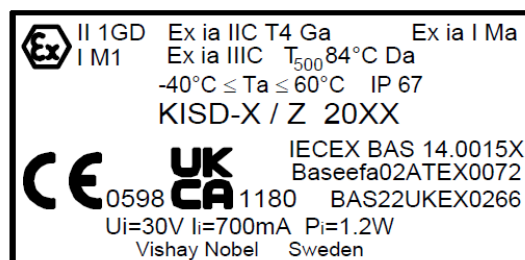


KISD

Functional safety

From a safety point of view is the KxxD-(D) load cell an individual safety component connected to an overall safety control unit. Each individual amplifier strain gauge bridge output shall be connected to separate control system input(s) as view in figure below, see also application examples.

For double channel system, cross monitoring of measurement signals is assumed to be implemented in the overall measuring instrument. The hardware reliability figures for the double channel load cell are valid when the overall measuring instrument is fulfilling correct monitoring of the load cell(s).

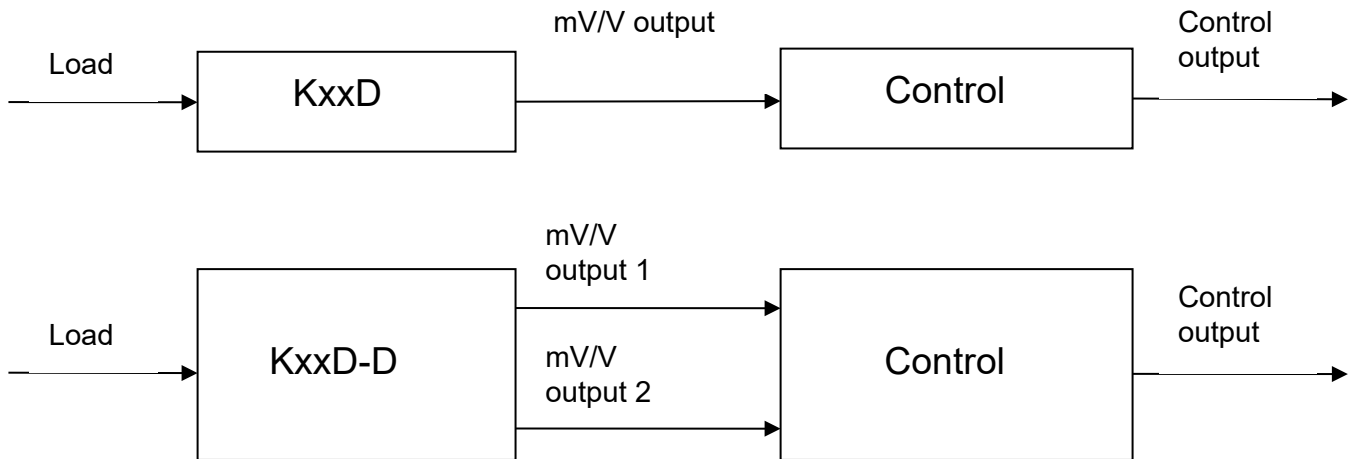

KxxD load cell safety parameters

According to EN ISO 13849-1:

- Category = 1
- MTTF_d = 48 year
- Maximum performance level, PL = c

KxxD-D load cell safety parameters

1. According to EN ISO 13849-1:

- Category = 3
- MTTF_d = 48 year
- Maximum performance level, PL = d

The achievable performance level assumes that the double channel load cell shall be connected to an overall measuring instrument in a category 3 structure with a diagnostic coverage, DC ≥ 90%. (Value of DC level is according to Annex E, table E.1). The comparison tolerance must be selected with respect to the specified element safety function.

2. According to EN 61508 with DC Low

- HFT = 1
- SFF = 80%
- PFH = $1.16 \cdot 10^{-8}$
- $\lambda_s = 1,20 \cdot 10^{-6}$
- $\lambda_{dd} = 7,21 \cdot 10^{-7}$
- $\lambda_{du} = 4,80 \cdot 10^{-7}$
- Maximum SIL = 2

3. According to EN 61508 with DC High

- HFT = 1
- SFF = 99.5%
- PFH = $2,41 \cdot 10^{-10}$
- $\lambda_s = 1,20 \cdot 10^{-6}$
- $\lambda_{dd} = 1,19 \cdot 10^{-6}$
- $\lambda_{du} = 1,20 \cdot 10^{-8}$
- Maximum SIL = 2

The overall measurement system (control) must implement the following diagnostic technique: "Input comparison/voting (1oo2, 2oo3 or better redundancy)" with DC = Low (60%) or DC = High (99%) according to IEC 61508-2 Table A.13. The comparison tolerance must be selected with respect to the specified element safety function.

Load cell connection

The load cell single or double strain gauge bridge outputs shall be connected using shielded cable. It shall then be connected to the measuring equipment bridge mV/V input signal channel.

The bridge power shall be connected to E+ and E- outputs and the measuring equipment signal input shall be connected to the S+ and S- outputs.

The cable should be routed at least 100 mm from other cables, so that electromagnetic interference is avoided. Cable shield is not connected to the load cell body and shall be grounded in the other end. The load cell connector housing is connected to the load cell body and the cable shield shall not be connected in the cable connector but be grounded in the other end. Cable shield is then grounded in one point only.


For installation in an explosive gas/dust or mining area, only trained personnel may perform dimensioning of cables and barriers. A descriptive system document should be prepared by the system designer.

Connector pin-out and wires color code:	
<u>Electrical connection</u>	
Connector type: (M12 or equivalent IP67 qualified)	
Cable: Shielded 4 or 8-wire 0,25mm ² cable through IP67 qualified cable gland	
<u>Connector pin number *</u>	<u>Cable: Cable wire colour *</u>
Pin 1: E+ (positive excitation). Bridge 1	Red: E+ (positive excitation). Bridge 1
Pin 3: S+ (positive signal). Bridge 1	Green: S+ (positive signal). Bridge 1
Pin 2: S- (negative signal). Bridge 1	White: S- (negative signal). Bridge 1
Pin 4: E- (negative excitation). Bridge 1	Grey: E- (negative excitation). Bridge 1
Pin 5: E+ (positive excitation). Bridge 2	Brown: E+ (positive excitation). Bridge 2
Pin 7: S+ (positive signal). Bridge 2	Blue: S+ (positive signal). Bridge 2
Pin 6: S- (negative signal). Bridge 2	Yellow: S- (negative signal). Bridge 2
Pin 8: E- (negative excitation). Bridge 2	Pink: E- (negative excitation). Bridge 2


* Deviations may occur in customer specific types.

Application examples

Load cell KxxD (one strain gauge bridge) and KxxD-D (two strain gauge bridges), used in a **non-hazardous** area, are shown below.

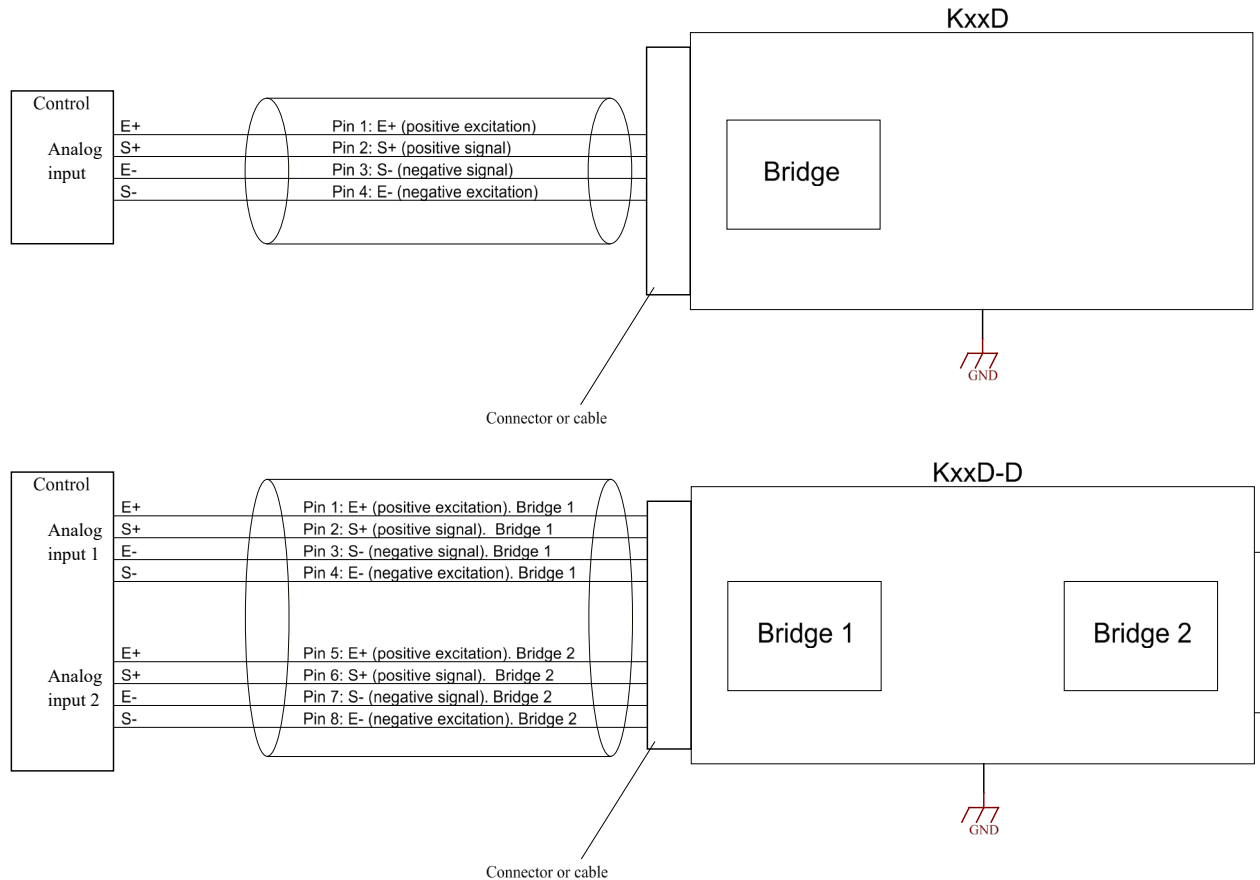

Load cell KxxD-D used in **hazardous** area is shown below. The cable shield is not connected to the load cell body and shall be connected in the other end. Connection to barrier or isolating IS unit is shown in the example below.

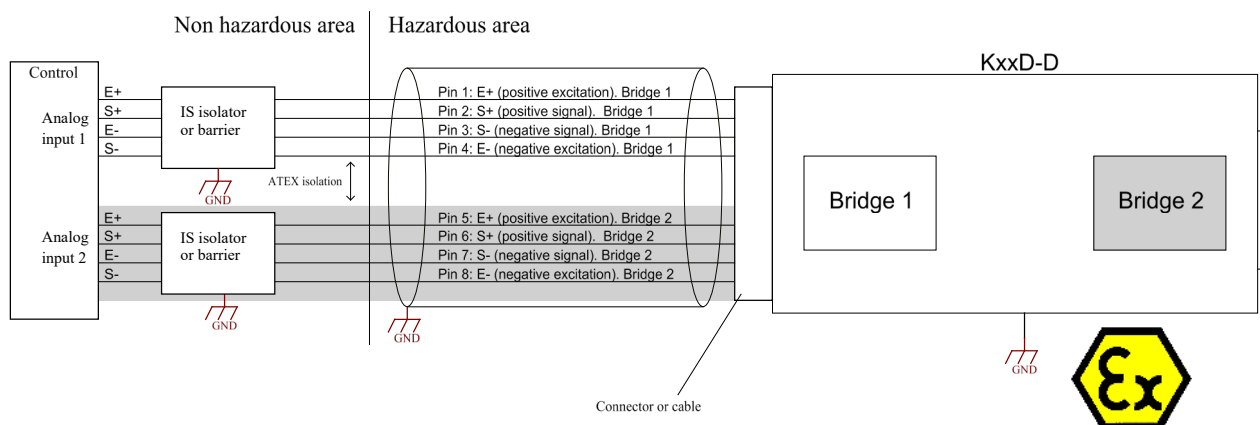

Load cell as a safety component can be used in both **hazardous** and **non-hazardous** areas and be connected to the measuring control in the same way.

Mechanical installation and maintenance

Load cells of the line KxxD-(D) are designed to be supported at both ends and loaded at the middle of the cylindrical body (KIMD, KOSD and KISD). An arrow on one or both ends define the correct direction of the resulting force from the applied load.

At the cable/connector end of the load cell, a flat reference surface or key slot are provided (KIMD, KOSD and KISD). It should be used to prevent the cylindrical load cell body from rotating in the supports.

Standardized adapters for some load cell types are available, others can be custom designed and produced by Vishay Nobel. On request the mechanical shape of a load cell can also be altered to suit an existing structure.

Potential electrostatic hazard on KIMD-(D), do not rub with electrostatic materials.



Potential electrostatic hazard on KIMD-(D), do not rub with electrostatic materials.

Mechanical data

KxxD-(D) series of load cells are often custom made for specific applications. For complete mechanical data on these load cells, refer to the detailed technical specification.

Appendix 1, 200418r5, Baseefa02ATEX0072

Certificate Number
Baseefa02ATEX0072
Issue 5



Issued 10 September 2025
Page 1 of 4

1 EU - TYPE EXAMINATION CERTIFICATE

2 Equipment or Protective System Intended for use in Potentially Explosive Atmospheres Directive 2014/34/EU

3 EU - Type Examination Certificate Number: **Baseefa02ATEX0072 – Issue 5**

3.1 In accordance with Article 41 of Directive 2014/34/EU, EC-Type Examination Certificates referring to 94/9/EC that were in existence prior to the date of application of 2014/34/EU (20 April 2016) may be referenced as if they were issued in accordance with Directive 2014/34/EU. Supplementary Certificates to such EC-Type Examination Certificates, and new issues of such certificates, may continue to bear the original certificate number issued prior to 20 April 2016.

4 Product: **Load Cell KXXD-X with variants**

5 Manufacturer: **Vishay Nobel AB**

6 Address: **Box 423, SE-691 27 Karlskoga, Sweden**

7 This re-issued certificate extends EC Type Examination Certificate No. Baseefa02ATEX0072 to apply to product designed and constructed in accordance with the specification set out in the Schedule of the said certificate but having any variations specified in the Schedule attached to this certificate and the documents therein referred to.

8 SGS Fimko Oy, Notified Body number 0598, in accordance with Article 17 of Directive 2014/34/EU of the European Parliament and of the Council, dated 26 February 2014, certifies that this product has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of products intended for use in potentially explosive atmospheres given in Annex II to the Directive.

8.1 The original certificate was issued by SGS Baseefa Ltd (UK Notified Body 1180). It, and any supplements previously issued by SGS Baseefa Ltd have been transferred to the supervision of SGS Fimko Oy (EU Notified Body 0598). The original certificate number is retained.

The examination and test results are recorded in confidential Report No. **See Certificate History**

9 Compliance with the Essential Health and Safety Requirements has been assured by compliance with:

EN IEC 60079-0:2018 EN 60079-11:2012

except in respect of those requirements listed at item 18 of the Schedule.

10 If the sign "X" is placed after the certificate number, it indicates that the product is subject to the Specific Conditions of Use specified in the schedule to this certificate.

11 This EU - TYPE EXAMINATION CERTIFICATE relates only to the design and construction of the specified product. Further requirements of the Directive apply to the manufacturing process and supply of this product. These are not covered by this certificate.

12 The marking of the product shall include the following:

Ⓢ II 1 GD Ex ia IIC T4 Ga Ex ia IIIC T₅₀₀ 84°C Da (-40°C ≤ Ta ≤ 60°C)

Ⓢ I M1 Ex ia I Ma (-40°C ≤ Ta ≤ 60°C)

SGS Fimko Oy Customer Reference No. **2054**

Project File No. **25/0464**

This document is issued by the Company subject to their General Conditions for Certification Services accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of their intervention only and within the limits of Client's instructions, if any. It does not necessarily indicate that the equipment may be used in particular industries or circumstances. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, schedule included, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS Fimko Oy

Takomotie 8

FI-00380 Helsinki, Finland

Telephone +358 9 696 361

www.sgs.com

Business ID 0634247-4 Member of the SGS
Group (SGS SA)



Mikko Välimäki
SGS Fimko Oy



13

Schedule

14

Certificate Number Baseefa02ATEX0072 – Issue 5

15 Description of Product

The Loadcells Type KXXD-X are designed to measure force. Each loadcell comprises a printed circuit board, four dual element strain gauges and two modulus gauges all housed in a stainless steel enclosure. External connections are made via an integral four core cable.

This certificate covers types KOSD-XXX-Z, KOSD-X, KOSD-New Style, KISD-X, KIMD-X and KXXD-DX, where X represents type and load rating and the -DX suffix represents a double-bridge type.

The apparatus comprises a stainless steel body, in which the strain and modulus gauges and the printed circuit board (coated with silicon rubber compound or varnish) are mounted. Electrical connections are made via a glanded integral cable, the termination of which, on the internal printed circuit board is encapsulated.

The loadcells are adequately protected against dust ingress; the enclosures offering a degree of protection of not less than IP6X.

Input Parameters

U_i	=	30V	C_i	=	See table below
I_i	=	1A	L_i	=	See table below
P_i	=	1.2W	L_i/R_i	=	See table below

Cable length	Capacitance, C_i	Inductance, L_i	L_i / R_i Ratio
< 10m	3.5nF	<10μH	30μH/Ω
>10m to 17m	5nF	<17μH	30μH/Ω
>17m to 25m	8nF	Use L_i/R_i ratio	30μH/Ω
>25m to 50m	15nF	Use L_i/R_i ratio	30μH/Ω
>50m to 100m	30nF	Use L_i/R_i ratio	30μH/Ω

16 Report Number

See Certificate History

17 Specific Conditions of Use

None

18 Essential Health and Safety Requirements

In addition to the Essential Health and Safety Requirements (EHSRs) covered by the standards listed at item 9, the following are considered relevant to this product, and conformity is demonstrated in the report:

Clause	Subject
1.2.7	Protection against other hazards (LVD type requirements, etc.)
1.2.8	Overloading of equipment (protection relays, etc.)
1.4.1	External effects
1.4.2	Aggressive substances, etc.

Certificate Number
Baseefa02ATEX0072
Issue 5



Issued 10 September 2025
Page 3 of 4

19 Drawings and Documents

New drawings submitted for this issue of certificate:

None.

Current drawings which remain unaffected by this issue:

Number	Sheet	Issue	Date	Description
300138	1 of 1	3	2022-10-05	KIMD Type Double Bridge Connector or Cable
300139	1 of 1	3	2022-10-05	KOSD Type Double Bridge Connector or Cable
300279	1 of 1	1	10-10-2002	KISD-X
300280	1 of 1	1	10-10-2002	KIMD-X ATEX
300331	1 of 1	1	10-10-2002	KOSD-XXX-Z ATEX
300332	1 of 1	5	2022-10-05	KOSD-New Style
400774	1 of 1	1	10-10-2002	KOSD-X ATEX
600610	1 of 1	6	2022-10-05	ATEX Label KOSD-X
600631	1 of 1	6	2022-10-05	ATEX Label KISD-X
600632	1 of 1	6	2022-10-05	ATEX Label KIMD-X
600633	1 of 1	6	2022-10-05	ATEX Label KOSD-XXX-Z

All drawings are held with IECEx BAS 14.0015X and are common to BAS22UKEX0266.

20 Certificate History

Certificate No.	Date	Comments
Baseefa02ATEX0072	18 October 2002	The release of the prime certificate. The associated test and assessment is documented in Test Report No.. Project File No. 02/0290.
Baseefa02ATEX0072/1	19 January 2010	To introduce the KXXD-DX double-bridge loadcell, to permit a change to the ambient temperature range to $-40^{\circ}\text{C} \leq T_a \leq +60^{\circ}\text{C}$, to confirm that the equipment covered by this certificate has been reviewed against the requirements of EN 60079-0:2009 and EN 60079-11:2007 in respect of the differences from EN 50014:1997 + Amds 1 & 2 and EN 50020:2002 and to confirm that the equipment covered by this certificate has been additionally reviewed against the requirements of IEC 60079-31:2008 and may also therefore be coded: Ex II 1D Ex t IIIC T80°C T₅₀₀84°C Da Project File No. 10/0535.
Baseefa02ATEX0072 Issue 2	11 November 2014	This issue of the certificate incorporates previously issued primary & supplementary certificates into one certificate and confirms the current design meets the requirements of EN 60079-0: 2012 & EN 60079-11: 2012 including the revision of the marking in accordance with these standards. IEC 60079-31:2008 has been removed and the code changed from Ex t IIIC to Ex ia IIIC. Ex II 1GD Ex ia IIC T4 Ga Ex ia IIIC T80°C T₅₀₀84°C Da The equipment has been assessed against the requirements for Group I and may also therefore be additionally coded: Ex I M1 Ex ia I Ma Test Report No. GB/BAS/ExTR14.0154/00. Project File No. 13/0709.
Baseefa02ATEX0072 Issue 3	11 June 2018	To permit a change in U_i from 25V to 30V (the parameters have been updated accordingly) and to confirm that the equipment meets the requirements of EN 60079-0: 2012+A11:2013. Test Report No. GB/BAS/ExTR18.0071/00. Project File No. 18/0220.

Certificate Number
Baseefa02ATEX0072
Issue 5



Issued 10 September 2025
Page 4 of 4

Certificate No.	Date	Comments
Baseefa02ATEX0072 Issue 4	12 April 2023	To confirm the current design meets the requirements of EN IEC 60079-0:2018. Test Report No: GB/BAS/ExTR23.0022/00 Project File No: 22/0544
Baseefa02ATEX0072 Issue 5	10 September 2025	To correct input parameter Li (inductance of attached cable). Project File No: 25/0464
For drawings applicable to each issue, see original of that issue.		

Appendix 2, 200706r1, BAS22UKEX0266

Certificate Number
BAS22UKEX0266
Issue 1



Issued 10 September 2025
Page 1 of 3

1 UK-TYPE EXAMINATION CERTIFICATE

2 **Equipment or Protective System Intended for use in Potentially Explosive Atmospheres**
UKSI 2016:1107 (as amended) – Schedule 3A, Part 1

3 UK-Type Examination Certificate Number: **BAS22UKEX0266 Issue 1**

4 Product: **Load Cell KXXD-X with variants**

5 Manufacturer: **Vishay Nobel AB**

6 Address: **Box 423, SE-691 27 Karlskoga, Sweden**

7 This product and any acceptable variation thereto is specified in the schedule to this certificate and the documents therein referred to.

8 SGS Baseefa, Approved Body number 1180, in accordance with Regulation 43 of the Equipment and Protective Systems Intended for Use in Potentially Explosive Atmospheres Regulations 2016, UKSI 2016:1107 (as amended), certifies that this product has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of products intended for use in potentially explosive atmospheres given in Schedule 1 of the Regulations.

8.1 The BAS prefix to the Certificate Number indicates that the certificate was issued by SGS Baseefa Ltd. prior to the change of entity to SGS United Kingdom Limited. Such certificates remain valid with their original number.

The examination and test results are recorded in a confidential report identified in the revision table at item 20.

9 Compliance with the Essential Health and Safety Requirements has been assured by compliance with:

EN IEC 60079-0:2018 EN 60079-11:2012

except in respect of those requirements listed at item 18 of the Schedule.

10 If the sign “X” is placed after the certificate number, it indicates that the product is subject to the Specific Conditions of Use specified in the schedule to this certificate.

11 This UK-TYPE EXAMINATION CERTIFICATE relates only to the design and construction of the specified product. Further requirements of the Regulations apply to the manufacturing process and supply of this product. These are not covered by this certificate.

12 The marking of the product shall include the following:

⊕ II 1 GD Ex ia IIC T4 Ga Ex ia IIIC T₅₀₀ 84°C Da (-40°C ≤ Ta ≤ 60°C)

⊕ I M1 Ex ia I Ma (-40°C ≤ Ta ≤ 60°C)

SGS Baseefa Customer Reference No. **2054**

Project File No. **25/0464**

This document is issued by the Company subject to its General Conditions for Certification Services accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and the Supplementary Terms and Conditions accessible at <http://www.sgs.com/SGSBaseefa/Terms-and-Conditions.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. It does not necessarily indicate that the equipment may be used in particular industries or circumstances. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, schedule included, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

SGS United Kingdom Ltd.

(Incorporating Baseefa Ltd.)

Rockhead Business Park, Staden Lane,

Buxton, Derbyshire SK17 9RZ

Telephone +44 (0) 1298 766600

e-mail baseefa@sgs.com web site www.sgs.co.uk/sgsbaseefa

Registered in England No. 01193985.

Registered address: Rossmore Business Park, Ellesmere Port, Cheshire, CH65 3EN



Authorised Signatory

13

Schedule

14

Certificate Number BAS22UKEX0266 Issue 1

15 Description of Product

The Loadcells Type KXXD-X are designed to measure force. Each loadcell comprises a printed circuit board, four dual element strain gauges and two modulus gauges all housed in a stainless steel enclosure. External connections are made via an integral four core cable.

This certificate covers types KOSD-XXX-Z, KOSD-X, KOSD-New Style, KISD-X, KIMD-X and KXXD-DX, where X represents type and load rating and the -DX suffix represents a double-bridge type.

The apparatus comprises a stainless steel body, in which the strain and modulus gauges and the printed circuit board (coated with silicon rubber compound or varnish) are mounted. Electrical connections are made via a glanded integral cable, the termination of which, on the internal printed circuit board is encapsulated.

The loadcells are adequately protected against dust ingress; the enclosures offering a degree of protection of not less than IP6X.

Input Parameters

U_i	=	30V	C_i	=	See table below
I_i	=	1A	L_i	=	See table below
P_i	=	1.2W	L_i/R_i	=	See table below

Cable length	Capacitance, C_i	Inductance, L_i	L_i / R_i Ratio
< 10m	3.5nF	<10 μ H	30 μ H/ Ω
>10m to 17m	5nF	<17 μ H	30 μ H/ Ω
>17m to 25m	8nF	Use L_i/R_i ratio	30 μ H/ Ω
>25m to 50m	15nF	Use L_i/R_i ratio	30 μ H/ Ω
>50m to 100m	30nF	Use L_i/R_i ratio	30 μ H/ Ω

16 Report Number

None.

17 Specific Conditions of Use

None

18 Essential Health and Safety Requirements

In addition to the Essential Health and Safety Requirements (EHSRs) covered by the standards listed at item 9, the following are considered relevant to this product:

Clause	Subject	Compliance
13	Protection against other hazards (LVD type requirements, etc.)	Standards require manufacturer's declaration, supplied.
14	Overloading of equipment (protection relays, etc.)	Covered by installation rules and manufacturer's instructions
21(1)	External effects	The Purchaser should make the manufacturer aware of such issues.
21(2)	Aggressive substances, etc.	The Purchaser should make the manufacturer aware of such issues.

Certificate Number
BAS22UKEX0266
Issue 1



Issued 10 September 2025
Page 3 of 3

19 Drawings and Documents

Other than for Issue 0, Drawings and Documents that are introduced at a new edition of the certificate are marked with an asterisk symbol:

Number	Sheet	Issue	Date	Description
300138	1 of 1	3	2022-10-05	KIMD Type Double Bridge Connector or Cable
300139	1 of 1	3	2022-10-05	KOSD Type Double Bridge Connector or Cable
300332	1 of 1	5	2022-10-05	KOSD-New Style
600610	1 of 1	6	2022-10-05	ATEX Label KOSD-X
600631	1 of 1	6	2022-10-05	ATEX Label KISD-X
600632	1 of 1	6	2022-10-05	ATEX Label KIMD-X
600633	1 of 1	6	2022-10-05	ATEX Label KOSD-XXX-Z

Refer to Baseefa02ATEX0072 Issue 5 for the full list of applicable drawings.

20 Certificate History

Certificate No.	Date	Comments
BAS22UKEX0266 Issue 0	12 April 2023	Prime Certificate Report Number: GB/BAS/ExTR23.0022/00 Project Number: 22/0544 Original issue of the certificate
BAS22UKEX0266 Issue 1	10 September 2025	This issue of the certificate corrects input parameters. Project Number No. 25/0464.
For drawings applicable to each issue, see original of that issue.		

Appendix 3, 200441r8, Declaration of Conformity

Declaration of Conformity

We Vishay Nobel AB
P.O. Box 423, SE-691 27 KARLSKOGA
Skrantahöjdsvägen 40, SE-691 46 KARLSKOGA
SWEDEN
declare under our sole responsibility that the products

**Load Cell KXXD-X with variants
(KOSD-XXX-Z, KOSD-X, KOSD-New Style, KISD-X, KIMD-X, KOSD-DX and KIMD-DX)**

to which this declaration relates are in conformity with the following standards
or other normative documents:

The essential requirements for safety component in the Machine Directive 2006/42/EC
EN ISO 13849-1:2015. KxxD up to PLc and KxxD-D up to PLd
EN 61508:2010. KxxD-D up to SIL 2
Function safety Certificate: TÜV 968/FSP 1462.00/17

The essential requirements in the EMC Directive 2014/30/EU
EN 61326-1:2013

The essential requirements in the ATEX Directive 2014/34/EU with later amendments
EN IEC 60079-0: 2018
EN 60079-11: 2012

Group I Category M1: Ex ia I Ma
Group II Category 1 GD: Ex ia IIC T4 Ga, Ex ia IIIC T₅₀₀84°C Da

EC – Type examination Certificate: Baseefa02ATEX0072
IEC – Type examination Certificate: IECEx BAS 14.0015X
UKCA – Type Certificate: BAS22UKEX0266

Notified Body for EC type examination / production: SGS Fimko Oy, NB No. 0598,
Helsinki FINLAND
Notified Body for UKCA production: SGS Baseefa Limited, NB No. 1180, Buxton UK

The essential requirements in the RoHS Directive 2011/65/EU Restriction of the use of certain
hazardous substances in electrical and electronic equipment.
EN 50581:2012

The product is supplied by up to 30 VDC/VAC and is therefore not covered by the requirements in
the Low Voltage Directive 2014/35/EU.

On behalf of the above named company, I declare that, on the date the equipment accompanied
by this declaration is placed on the market, the equipment conforms with all technical and
regulatory requirements of the above listed directives.

KARLSKOGA, 13th of October 2025



Per Fredriksson, Managing Director

Appendix 4, IECEx and Functional Safety Certificates

IECEx Certificate

The IECEx certificate for the KxxD (-D) Load cell can be found on the official IECEx web site:
<https://www.iecex.com/>

Certificate number: IECEx BAS 14.0015X Issue No. 4.
200498r4

Functional safety Certificate

The functional safety certificate for the KxxD (-D) Load cell can be found on TÜV Rheinland web site: www.fs-products.com and www.certipedia.com/fs-products

Certificate number: 968/FSP 1462.01/22

Publication: 600659R10
© Vishay Nobel AB, 2025-10-13
Subject to changes without notice.

Vishay Nobel AB
Box 423, SE-691 27 Karlskoga, Sweden
Phone +46 586 63000
blhnobel.se@vpgsensors.com
www.blhnobel.com